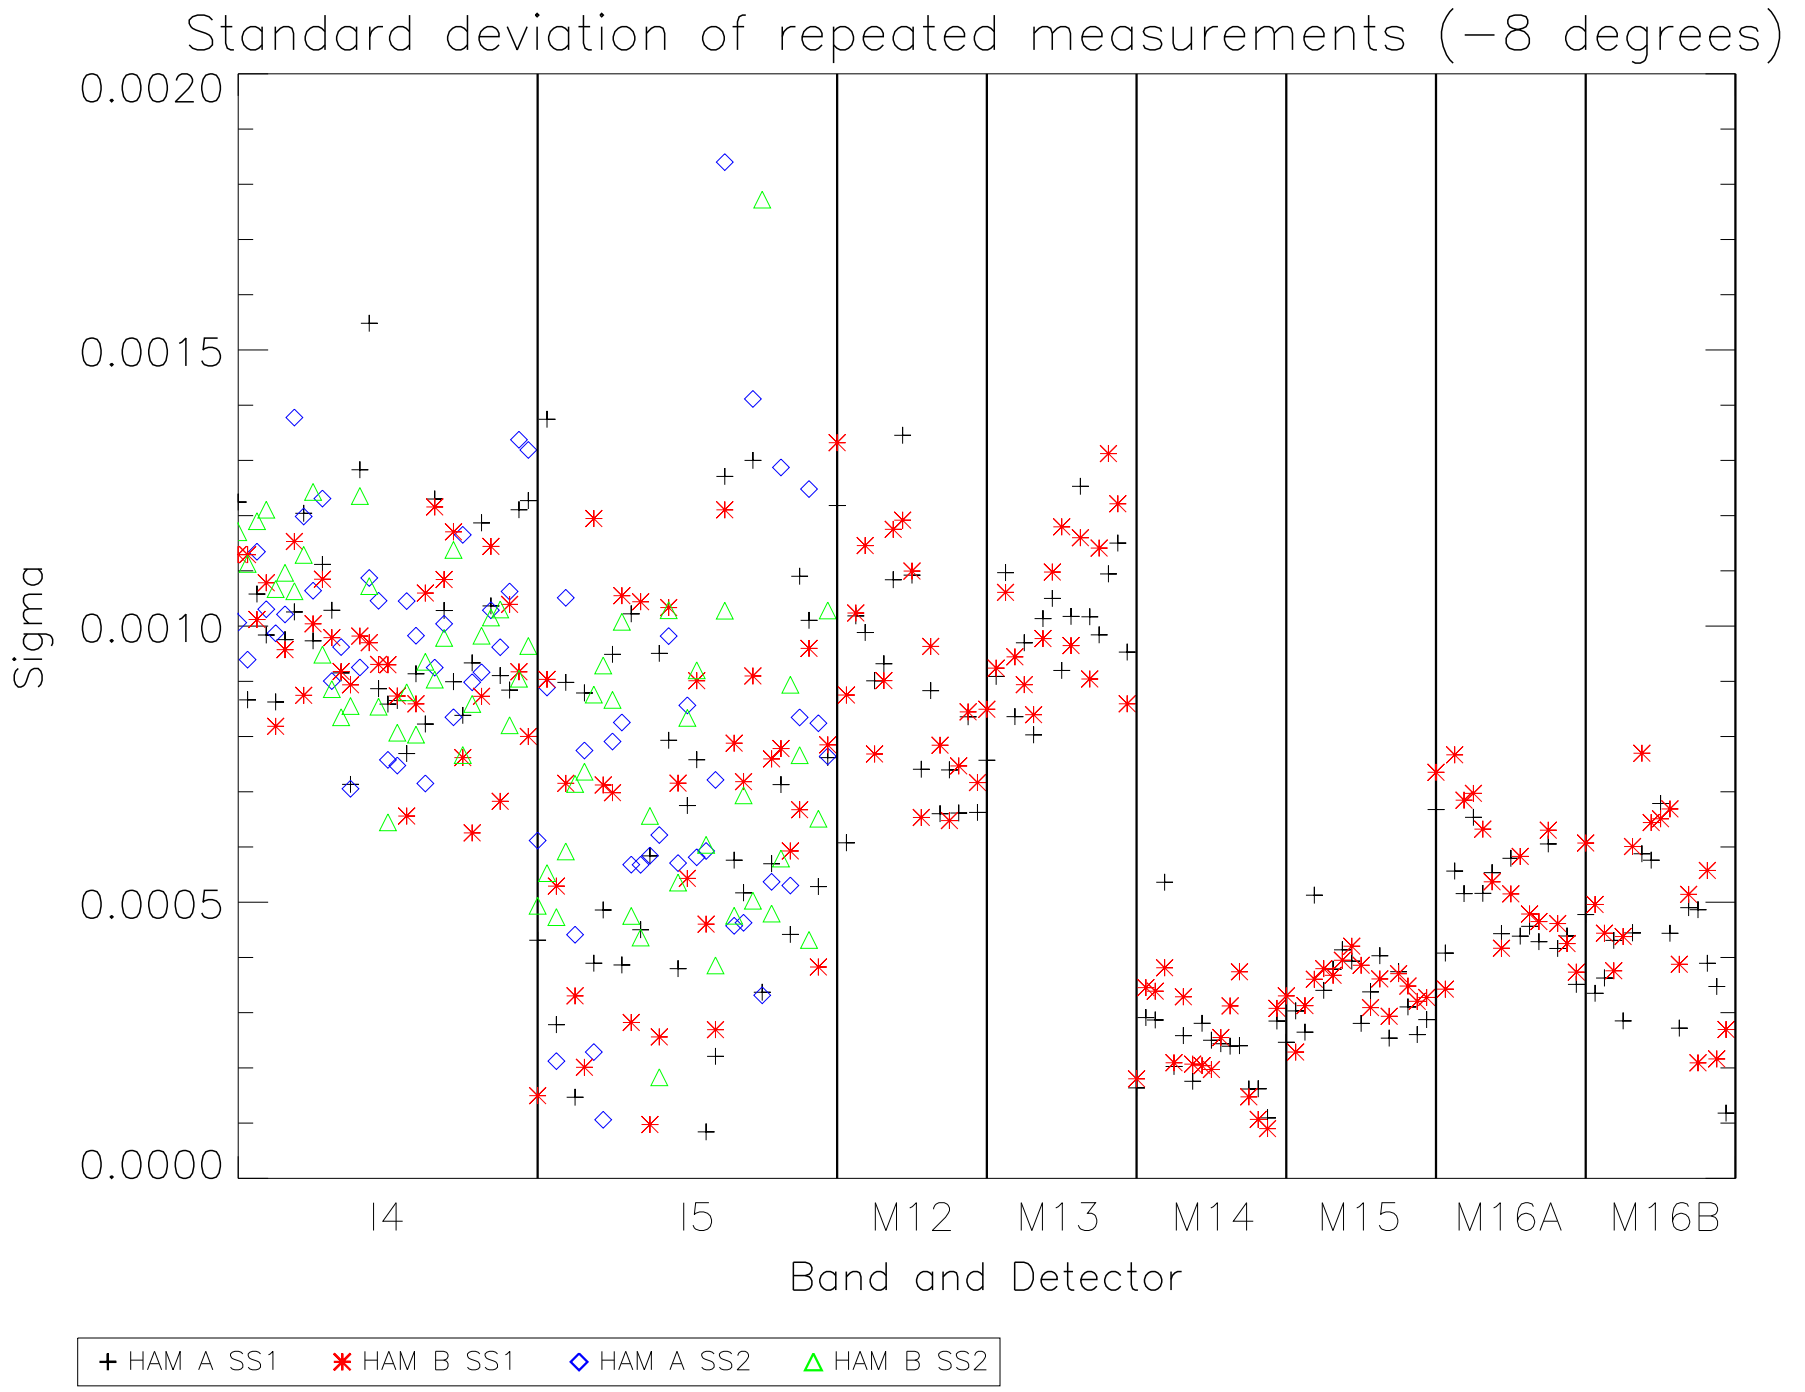
Standard deviation of repeated measurements (−8 degrees)
Sigma
0.0020
0.0015
0.0010
0.0005
0.0000
I4
I5
M12
M13
M14
M15
M16A
M16B
Band and Detector
HAM A SS1
HAM B SS1
HAM A SS2
HAM B SS2